



Patient Safety Checklist

Oxygenation Monitoring During In-Hospital Transport For Neonates and Infants


Patient Name: _____ Date: _____
Pt. floor/Rm #: _____ Destination: _____ Time: _____ AM/PM

PATIENT READINESS FOR TRANSPORT

- Respiratory Rate: _____ Heart Rate: _____
- Observed SpO₂ level at outset: _____ %
- Target SpO₂ range _____
 < 32 wks GA SpO₂ range 85–92%
 33–38 wks GA SpO₂ range 86–94%
 > 38 wks GA SpO₂ range 92–97%
- If applicable, supplemental oxygen @ _____ L/min (FiO₂ @ _____) via:
 Nasal cannula Incubator Oxyhood
- Breathing pattern:
 Regular Irregular Shallow Rapid
 Retractions: Yes No Nasal Flaring: Yes No
- Color: Pink Pale Dusky Cyanotic

MONITORING EQUIPMENT – DEVICE READINESS

- Alarm parameters
 Low SpO₂ alarm set @ _____ %
 High SpO₂ alarm set @ _____ %
- Pulse Oximeter:
 Monitor, sensor and connecting cables in good physical condition
 All controls operate as intended
 All audio and visual alarms functional
- Battery charge: Full 75%
 50% ≤ 50%
- Sensor placement: Circle location

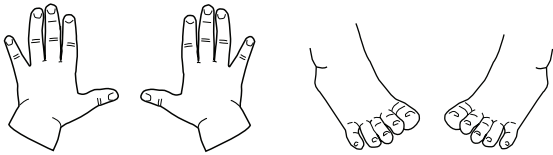

- Earlobe: right left
- Forehead Other: _____
- Sensor is attached to patient and secured for transport

OXYGEN SUPPLY

- Estimated duration of transport:
 < ½ hr ½ - 1 hr > 1 hr
- Sufficient oxygen for duration of transport

E Cylinder Duration Guide				
FLOW Liters per minute	500 PSIG 1/4 Full 155 liters	1000 PSIG 1/2 Full 310 liters	1500 PSIG 3/4 Full 465 liters	2000 PSIG Full 620 liters
0.5	5 hr.	10 hr.	15 hr.	20 hr.
1	2.5 hr.	5 hr.	7 hr. 45 min.	10 hr.
1.5	1 hr. 45 min.	3.4 hr.	5 hr.	6 hr. 45 min.
2	1 hr. 17 min.	2.5 hr.	3 hr. 50 min.	5 hr.
2.5	1 hr.	2 hr.	3 hr.	4 hr.
3	51 min.	1 hr. 50 min.	2.5 hr.	3 hr. 20 min.
4	38 min.	1 hr. 15 min.	1 hr. 55 min.	2.5 hr.
5	31 min.	1 hr.	1.5 hr.	2 hr.
6	25 min.	50 min.	1 hr. 17 min.	1hr. 40 min.
10	15 min.	30 min.	46 min.	1 hr.
15	10 min.	20 min.	30 min.	40 min.

- Circle estimated cylinder duration on chart
- Time oxygen cylinder started _____ AM/PM
- Estimated time of cylinder depletion: _____ AM/PM

References

Finer N, Leone T. Oxygen saturation monitoring for the pre-term infant: the evidence base for current practice. *Pediatr Res* 2009; Vol 65, No 4: 375-80.

Sahni R, Gupta A, Ohira-Kist K, Rosen TS. Motion resistant pulse oximeters in neonates. *Arch Dis Child Fetal Neonatal Ed* 2003; Vol 88, No 6; F 505-08.

Shiao SY, Ou CN. Validation of oxygen saturation monitoring in neonates. *Am J Crit Care* 2007; Vol 16, No 2; 168-78.

Sedaghat-Yazdi F, Torres A, Fortuna R, Geiss DM. Pulse oximetry accuracy and precision affected by sensor location in cyanotic children. *Pediatr Crit Care Med* 2008; Vol 9, No 4; 393-97.

Tin W, Walker S, Lacamp C. Oxygen monitoring in preterm babies: too high, too low? *Paediatr Respir Rev* 2003; Vol 4, No 1; 9-14.

Tluczek PS, et al. Effect of decreasing target oxygen saturation on retinopathy of prematurity. *J AAPOS* 2010. Oct; 14(5):406-11